

Phonak CROS B

User Guide



A Sonova brand

PHONAK
life is on

This user guide is valid for:

Wireless models

Phonak CROS B-312

Phonak CROS B-13

CE mark applied

2016

2016

ⓘ This user guide only applies to the CROS device.
Please see the hearing aid user guide for instructions
related to the hearing aid.



Your CROS device

i If no box is checked and you do not know the model of your CROS device, please ask your hearing care professional.

Model

CROS B-312

CROS B-13

Battery type

312

13

Earpiece

Dome or SlimTip

Classic earmold

Your CROS device has been developed by Phonak – the world leader in hearing solutions based in Zurich, Switzerland.

This premium product is the result of decades of research and expertise and is designed to keep you connected to the beauty of sound! We thank you for making such a great choice and wish you many years of listening pleasure.

Please read the User Guide carefully to make sure that you understand and get the best out of your CROS device. For more information about features and benefits, simply contact your hearing care professional.

Phonak - life is on
www.phonak.com

Contents

Your CROS device

- 1. Quick guide 6
- 2. Parts of the CROS device 8

Using the CROS device


- 3. Left & right CROS device markings 10
- 4. On/Off 11
- 5. Batteries 12
- 6. Putting on the CROS device 14
- 7. Removing the CROS device 16
- 8. Push button 18
- 9. Volume control 19

Further Information

- 10. Care and maintenance 20
- 11. Service and warranty 23
- 12. Compliance information 25
- 13. Information and description of symbols 29
- 14. Troubleshooting 32
- 15. Important safety information 34

1. Quick guide

Left & right markings



CROS B-312




CROS B-13


Blue marking for
left device.

Red marking for
right device.

Changing batteries



Remove the
sticker from the
new battery and
wait two minutes.




Open the
battery door.




Place battery in
the battery door
with the "+"
symbol facing
upwards.

On/Off




On




Off

Push button



The push button on your device can have various functions. The function is indicated in your individual instructions.

Volume control



CROS B-13 only:

To increase the volume, press the volume control upwards. To decrease the volume, press the volume control downwards.

2. Parts of the CROS device

The following pictures show the models described in this user guide. You can identify your personal model by:


- Checking "Your CROS device" on page 3.
- Or comparing your CROS device with the models shown on the following page. Pay attention to the shape of the hearing aid and if a volume control is present.

The Phonak CROS device is an application for single-sided deafness, one-sided hearing loss or asymmetrical hearing loss. It is placed on the impaired ear and wirelessly transmits sound to the Phonak hearing aid on the other ear.


Phonak CROS B device + Phonak hearing aid =
Phonak CROS system

i Phonak CROS B only works in connection with a Phonak Belong™ hearing aid as the receiver.

CROS B-312

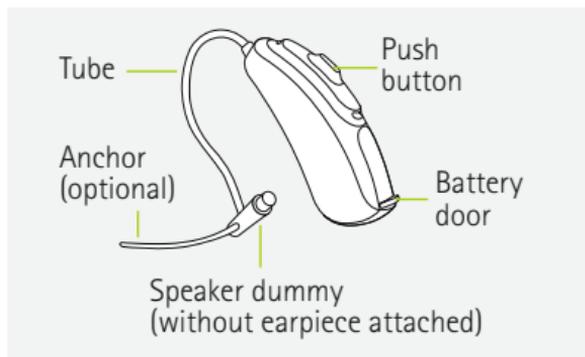

CROS B-13

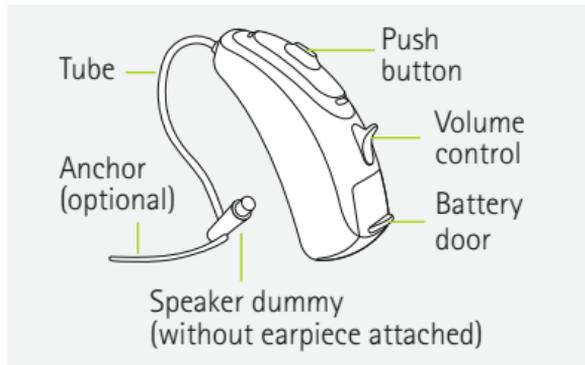

Possible earpieces for the CROS B device



Dome



SlimTip



Classic earmold*



* for CROS B-13 only

3. Left & right CROS device markings


There is a red or blue marking to tell you if it is a left or a right device.

CROS B-312 only:

To open the battery door, pull down the ridge at the bottom of the device.



CROS B-312



CROS B-13

Blue marking for
left device.


Red marking for
right device.

4. On/Off

The battery door is also the on/off switch.


1

Closed battery door =
CROS device is **on**

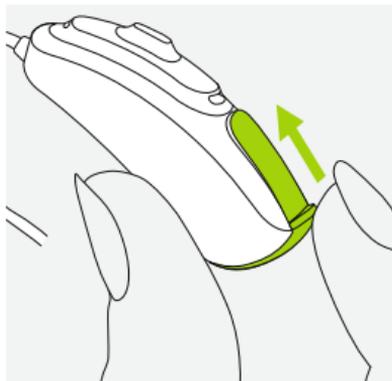


2


Open battery door =
CROS device is **off**

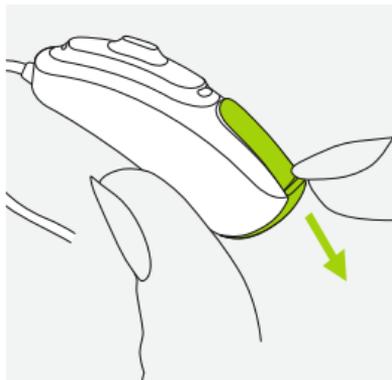


5. Batteries



Remove the sticker from the new battery and wait two minutes.



Open the battery door.



Place battery in the battery door with the "+" symbol facing upwards.

- ⓘ If it is difficult to close the battery door: Check that the battery is inserted correctly and the "+" symbol is facing the "+" label inside the battery compartment. If the battery is not inserted correctly, the CROS device will not work and the battery door can be damaged.

 Low power: You will hear two beeps followed by a melody  when the battery of the CROS device is low. You will have approximately 30 minutes to

change the battery (this can vary, depending on the battery). We recommend that you always have a new battery at hand.

Replacement battery

This CROS device requires zinc-air batteries. Identify the correct battery size (312 or 13) by:

- Checking "Your CROS device" on page 3.
- Checking the marking on the inner side of the battery door.
- Checking the following table.

Model	Zinc air battery size	Color marking on package	IEC code	ANSI code
CROS B-312	312	brown	PR41	7002ZD
CROS B-13	13	orange	PR48	7000ZD


 Please ensure you use the correct type of battery in your CROS device (zinc-air). Please also read chapter 15.2 for further information on product safety.

6. Putting on the CROS device

6.1 Putting on the CROS device with dome or SlimTip


1

Place the CROS device behind your ear.

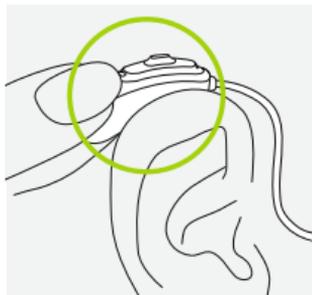


2

Insert the earpiece into your ear canal.

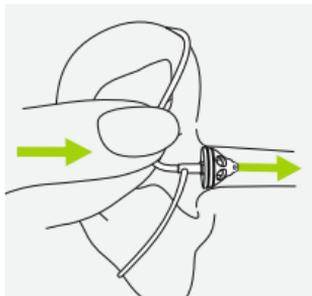

3


If there is an anchor attached to the earpiece, tuck it into the bowl of your ear to secure your CROS device.

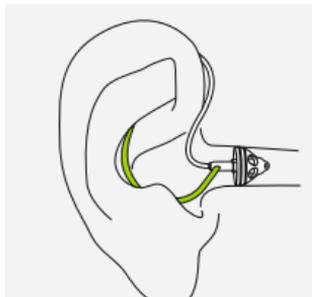

6.2 Putting on the CROS device with classic earmold


1

Take the earmold up to your ear and place the ear canal part into your ear canal.

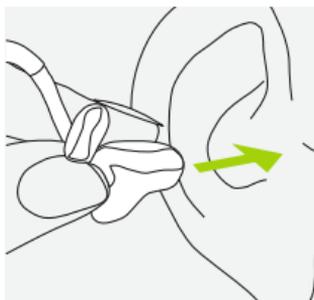


2

Place the CROS device behind your ear.

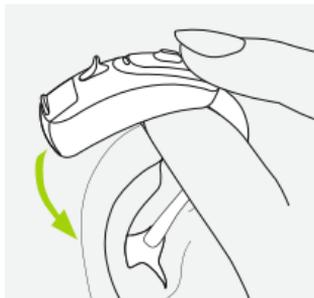

3

Insert the upper part of the earmold into the upper part of the bowl of your ear.

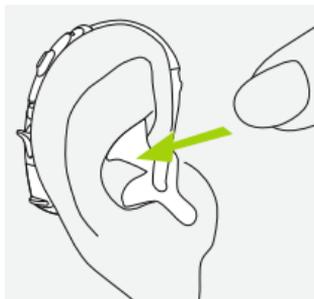


7. Removing the CROS device

7.1 Removing the CROS device with dome or SlimTip

1

Pull on the bend of the tube and remove the CROS device from behind the ear.

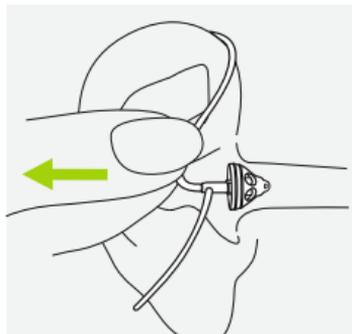


In very rare cases, your earpiece can remain in your ear canal when removing the device from the ear. In the unlikely case that the earpiece does get stuck in your ear canal, it is strongly recommended to see a medical specialist for safe removal.

7.2 Removing the CROS device with classic earmold


1

Lift the device above the upper part of your ear.

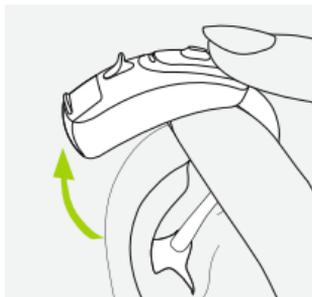

2


Grasp the earmold in your ear and gently remove it.

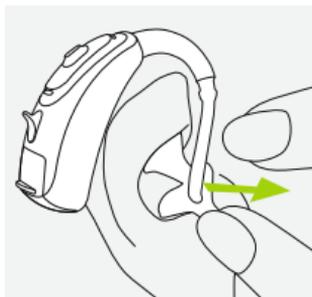

ⓘ Please try to avoid gripping the tube to remove the CROS device.

8. Push button

The push button on your CROS device can have various functions or is not active. This depends on the programming of the CROS device, which is indicated in your individual "Hearing aid instructions". Please ask your hearing care professional for this printout.

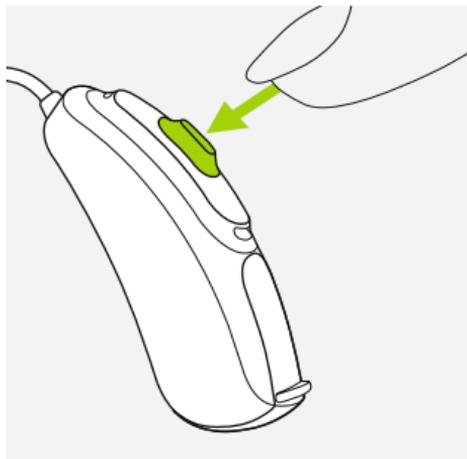

9. Volume control

CROS B-13 only:

To increase the volume, press the volume control upwards. To decrease the volume, press the volume control downwards.

The volume control of your CROS device can have various functions or is not active. This depends on the programming, which is indicated in your individual "Hearing aid instructions". Please ask your hearing care professional for this printout.



10. Care and maintenance

Diligent and routine care of your CROS device contributes to outstanding performance and a long service life.

Please use the following specifications as a guideline. Further information regarding product safety, see chapter 15.2.

General information

Before using hair spray or applying cosmetics, you should remove your CROS device from your ear, because these products may damage it.

When you are not using your CROS device, leave the battery door open so that any moisture can evaporate. Make sure that you always completely dry your CROS device after use. Store it in a safe, dry and clean place.

Your CROS device is resistant to water, sweat and dust under the following conditions:

- The battery door is fully closed. Ensure that no foreign object such as hair is caught in the battery door when it is closed.
- After exposure to water, sweat or dust, the device is cleaned and dried.
- The CROS device is used and maintained as described in this user guide.

ⓘ Use of your CROS device around water can restrict air flow to the batteries causing it to stop working. Should your CROS device stop working after coming into contact with water, refer to the troubleshooting steps in chapter 14.

Daily

Inspect the earpiece (dome or SlimTip) for earwax and moisture deposits. Clean the surfaces with a lint-free cloth or use the small brush provided in the hard case. Never use cleaning agents such as household detergents, soap, etc. for cleaning your CROS device. It is not recommended to rinse with water. If you need to clean your CROS device intensively, ask your hearing care professional for advice and information on drying capsules.

Weekly

Clean the earpiece (dome or SlimTip) with a soft, damp cloth or with a special cleaning cloth for hearing aids. For more in depth maintenance instructions or for more than basic cleaning, please see your hearing care professional.

Monthly

Inspect your tube for color changes, hardening, or cracks. In the case of such changes, the tube has to be replaced. Please see your hearing care professional.

11. Service and warranty

Local warranty

Please ask the hearing care professional, where you purchased your CROS device, about the terms of the local warranty.

International warranty

Phonak offers a one year limited international warranty, valid from the date of purchase. This limited warranty covers manufacturing and material defects in the CROS device itself, but not accessories such as batteries, tubes, earmolds, external receivers. The warranty only comes into force if a proof of purchase is shown.

The international warranty does not affect any legal rights that you might have under applicable national legislation governing sale of consumer goods.

Warranty limitation

This warranty does not cover damage from improper handling or care, exposure to chemicals or undue stress. Damage caused by third parties or non-authorized service centers renders the warranty null and void. This warranty does not include any services performed by a hearing care professional in their office.

Serial number:

Authorized hearing care
professional (stamp/signature):

Date of purchase:

12. Compliance information

Europe:

Declaration of Conformity

Hereby Phonak AG declares that this Phonak product meets the requirements of the Medical Devices Directive 93/42/EEC as well as the Radio and Telecommunications Terminal Equipment Directive 1999/5/EC. The full text of the Declaration of Conformity can be obtained from the manufacturer or the local Phonak representative whose address can be taken from the list on www.phonak.com (Phonak worldwide locations).

Australia/New Zealand:



R-NZ

Indicates a device's compliance with applicable Radio Spectrum Management's (RSM) and Australian Communications and Media Authority (ACMA) regulatory arrangements for the legal sale in New Zealand and Australia.

The compliance label R-NZ is for radio products supplied in the New Zealand market under conformity level A1.

The wireless models listed on page 2 are certified under:

Phonak CROS B-312

USA	FCC ID: KWC-WHSRIC2
Canada	IC: 2262A-WHSRIC2

Phonak CROS B-13

USA	FCC ID: KWC-WHSRIC4
Canada	IC: 2262A-WHSRIC4

Notice 1:

This device complies with Part 15 of the FCC Rules and with RSS-210 of Industry Canada. Operation is subject to the following two conditions:

- 1) this device may not cause harmful interference, and
- 2) this device must accept any interference received, including interference that may cause undesired operation.

Notice 2:

Changes or modifications made to this device not expressly approved by Phonak may void the FCC authorization to operate this device.

Notice 3:

This device has been tested and found to comply with the limits for a Class B digital device, pursuant to Part 15 of the FCC Rules and ICES-003 of Industry Canada. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This device generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful

interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this device does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the device and receiver.
- Connect the device into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

13. Information and description of symbols



With the CE symbol, Phonak AG confirms that this Phonak product – including accessories – meets the requirements of the Medical Devices Directive 93/42/EEC as well as the R&TTE Directive 1999/5/EC on radio and telecommunications equipment. The numbers after the CE symbol correspond to the code of certified institutions that were consulted under the above-mentioned directives.



This symbol indicates that the products described in these user instructions adhere to the requirements for an applied part of Type B of EN 60601-1. The surface of the hearing aid is specified as an applied part of Type B.



Indicates the medical device manufacturer, as defined in EU Directive 93/42/EEC.



During transportation keep dry.



This symbol indicates that it is important for the user to read and take into account the relevant information in these user guides.



This symbol indicates that it is important for the user to pay attention to the relevant warning notices in these user guides.



Important information for handling and product safety.

Operating conditions

The product is designed such that it functions without problems or restrictions if used as intended, unless otherwise noted in these user guides.



Indicates the manufacturer's serial number so that a specific medical device can be identified.



Indicates the manufacturer's catalogue number so that the medical device can be identified.



Temperature during transportation and storage: -20° to $+60^{\circ}$ Celsius (-4° to $+140^{\circ}$ Fahrenheit).



Humidity during transportation: Up to 90% (non condensing). Humidity during storage: 0% to 70%, if not in use. See instruction in chapter 15.2 regarding drying the device after use.



Atmospheric pressure: 200 hPa to 1500 hPa



The symbol with the crossed-out garbage bin is to make you aware that this device may not be thrown away as normal household waste. Please dispose of old or unused device, at waste disposal sites intended for electronic waste, or give your device to your hearing care professional for disposal. Proper disposal protects the environment and health.

14. Troubleshooting

Problem

CROS device not functioning

Causes

Flat battery

Battery not inserted correctly

CROS device switched off

Hearing aid switched off

Hearing aid plays two beeps

Indication for low hearing aid battery

Hearing aid plays two beeps followed by a melody 

Indication for low battery of CROS device

Sound switches on & off (intermittent)

Moisture on battery of hearing aid or CROS device

 If the problem persists, contact your hearing care professional for assistance

What to do

Change battery (chapter 1 + 5)

Insert battery correctly (chapter 1 + 5)

Switch CROS device on by completely closing the battery door (chapter 4)

Switch hearing aid on by completely closing the battery door (consult the user guide of the hearing aid if necessary)

Change battery of the hearing aid within the next 30 minutes (consult the user guide of the hearing aid if necessary)

Change battery of the CROS device within the next 30 minutes (chapter 1 + 5)

Wipe batteries and housing of the hearing aid and the CROS device with dry cloth

15. Important safety information

Please read the information on the following pages before using your CROS device.

A CROS device will not restore normal hearing and will not prevent or improve a hearing impairment resulting from organic conditions. Infrequent use does not permit a user to attain full benefit from it. The use of a CROS device is only part of hearing habilitation and may need to be supplemented by auditory training and instruction in lipreading.

15.1 Hazard warnings

-  The intended use of a CROS device is to transmit sound to a hearing aid on the better hearing ear and hereby compensate for impaired hearing. The CROS system (specially programmed for each hearing loss) must only be used by the intended person. It should not be used by any other person as it could damage hearing.
-  Changes or modifications to the CROS system that were not explicitly approved by Phonak are not permitted. Such changes may damage your ear or the CROS system.
-  Do not use the CROS system in explosive areas (mines or industrial areas with danger of explosions, oxygen rich environments or areas where flammable anesthetics are handled) or where electronic equipment is prohibited.
-  Hearing aid batteries are toxic if they are swallowed! Keep out of the reach of children, individuals with cognitive impairment, and pets. If batteries are swallowed, consult your physician immediately!

 If you feel pain in or behind your ear, if it is inflamed or if skin irritation and accelerated accumulations of earwax occur, please check with your hearing care professional or physician.

 In very rare cases, the earpiece can remain in your ear canal when removing the hearing tube from the ear. In the unlikely case that the earpiece does get stuck in your ear canal, it is strongly recommended to see a physician for safe removal.

 Hearing programs in the directional microphone mode reduce background noises. Please be aware that warning signals or noises coming from behind, e. g. cars, are partially or entirely suppressed.

 This CROS system is not for children below 36 months. It contains small parts that can cause choking, if swallowed by children. Keep out of the reach of children, individuals with cognitive impairment, and pets. If swallowed, consult a physician or hospital immediately.

 Do not make a wire connection from your hearing aid to any external audio sources like radio etc. That could cause injuries on your body (electric shock).

 The following is only applicable for persons with active implantable medical devices (i.e. pacemakers, defibrillators, etc.).

- Keep the wireless hearing aid or CROS device at least 15 cm (6 inches) away from the active implant. If you experience any interference, do not use the wireless hearing aids or CROS device and contact the manufacturer of the

active implant. Please note that interference can also be caused by power lines, electrostatic discharge, airport metal detectors etc.

- Keep magnets (i.e. battery handling tool, EasyPhone magnet, etc.) at least 15 cm (6 inches) away from the active implant.
- If using a Phonak wireless accessory, consult the chapter "Important safety information" in your wireless accessory user guide.

15.2 Information on product safety

- ① Phonak CROS devices are water resistant and not waterproof. They are designed to withstand normal activities and occasional accidental exposure to extreme conditions. Never immerse your CROS device in water! Phonak CROS devices are not specifically designed for extended periods of water submersion on a continual basis, that is worn in activities such as swimming or bathing. Always remove your CROS device before these activities, as the CROS devices contains sensitive electronic parts.
- ① Never wash the microphone inputs. Doing so could cause it to lose its special acoustic features.
- ① Protect your CROS device from heat (never leave near a window or in the car). Never use a microwave or other heating devices to dry your CROS device. Ask your hearing care professional about suitable drying methods.
- ① When you are not using your CROS device, leave the battery door open so that any moisture can evaporate. Make sure that you always completely dry

your CROS device after use. Store the CROS device in a safe, dry and clean place.

i Do not drop your CROS device! Dropping onto a hard surface can damage your CROS device.

i Always use new batteries for your CROS device. In case a battery is leaking, replace it immediately with a new one to avoid any skin irritation. You can return used batteries to your hearing care professional.

i The batteries used in the CROS device should not exceed 1.5 Volts. Please do not use silver-zinc or lithium-ion rechargeable batteries as these may cause severe damage to your CROS device. The table in chapter 5 explains exactly which type of battery your CROS device requires.

i Remove the battery if you are not using your CROS device for a long period of time.

① Special medical or dental examination including radiation described below, may adversely affect the correct functioning of your CROS device. Remove and keep them outside the examination room/area before undergoing:

- Medical or dental examination with X-ray (also CT scan).
- Medical examinations with MRI/NMRI scans, generating magnetic fields.
- CROS devices don't need to be removed when passing security gates (airports etc.). If X-ray is used at all, it will be in very low doses, and will not affect the CROS device.

Your hearing care professional:



029-0408-02/V1.00/2016-05/cu © Phonak AG All rights reserved



Manufacturer:

Phonak AG

Laubisrütistrasse 28

CH-8712 Stäfa

Switzerland

www.phonak.com



522721

613275

7

sonova
HEAR THE WORLD



0459